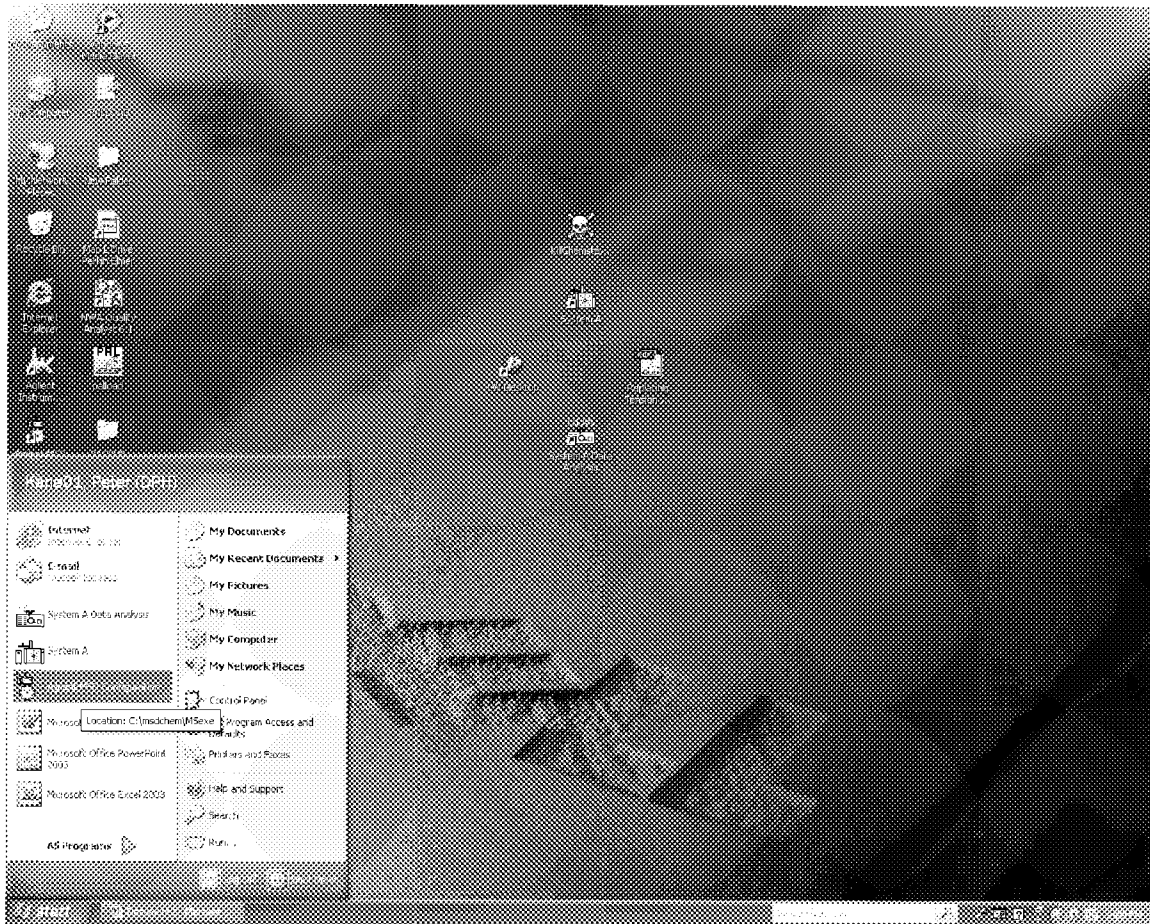1. Close down chemstation
2. Go to start and choose Agilent MSD Configuration

3. Right click on the Enviroquant option under the data analysis column and choose that instrument.

4. Under data analysis at the bottom of the screen that pops up choose Enhanced rather than Enviroquan.